



DREAM SLEEP RESPIRATORY SERVICES - CALGARY
 UNIT 222-5149 COUNTRY HILLS BLVD NW
 CALGARY
 Alberta, T3A 5K8

Phone: 403-457-1127
 Fax: 403-457-1288
 Email: troy@dreamsleep.ca

Howell, William

02/07/2019 - 04/07/2019

DOB: 02/25/1956

Age: 63 years


Compliance Report

Usage		02/07/2019 - 04/07/2019
Usage days		58/60 days (97%)
>= 4 hours		53 days (88%)
< 4 hours		5 days (8%)
Usage hours		400 hours 11 minutes
Average usage (total days)		6 hours 40 minutes
Average usage (days used)		6 hours 54 minutes
Median usage (days used)		7 hours 9 minutes
Total used hours (value since last reset - 04/07/2019)		484 hours

AirSense 10 AutoSet	
Serial number	23183362315
Mode	AutoSet
Min Pressure	7 cmH2O
Max Pressure	18 cmH2O
EPR	Fulltime
EPR level	3
Response	Standard

Therapy						
Pressure - cmH2O	Median:	10.6	95th percentile:	15.0	Maximum:	16.4
Leaks - L/min	Median:	0.0	95th percentile:	0.1	Maximum:	2.6
Events per hour	AI:	1.4	HI:	0.4	AHI:	1.8
Apnea Index	Central:	0.3	Obstructive:	1.0	Unknown:	0.0
RERA Index						0.1
Cheyne-Stokes respiration (average duration per night)						0 minutes (0%)

Usage - hours

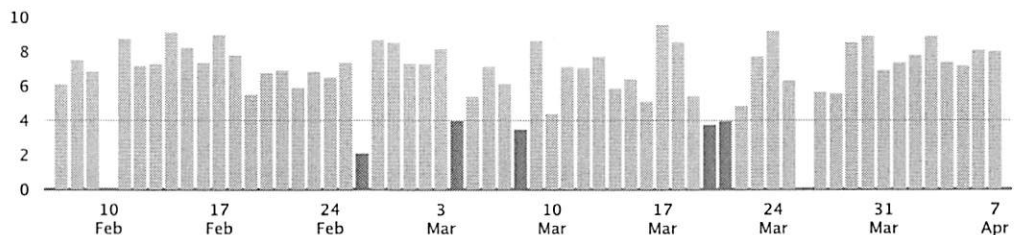



Phone: 403-457-1127
 Fax: 403-457-1288
 Email: troy@dreamsleep.ca

DOB: 02/25/1956
 Age: 63 years




Therapy Report

AirSense 10 AutoSet SN: 23183362315


Usage (hours)

Usage days **58/60 (97%)**
 >= 4 hour days **53 (98%)**
 < 4 hour days **5 (8%)**
 Days not used **2 (3%)**
 Days no data **0 (0%)**
 Used/day (avg.) **6.9 hrs.**

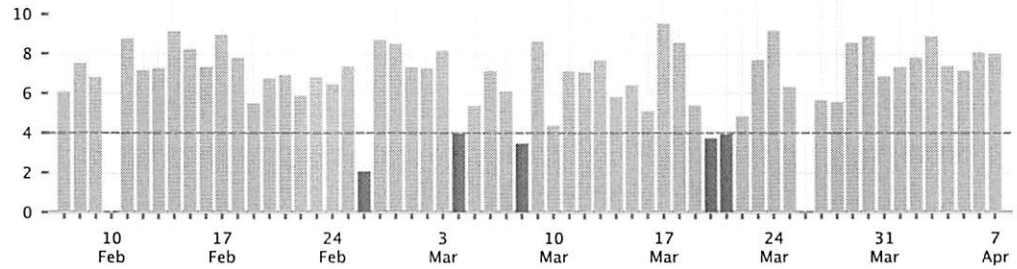


Leak (L/min)

Set threshold **24.0 L/min**
 Maximum (avg) **2.6**
 95th % (avg) **0.1**
 Median (avg) **0.0**

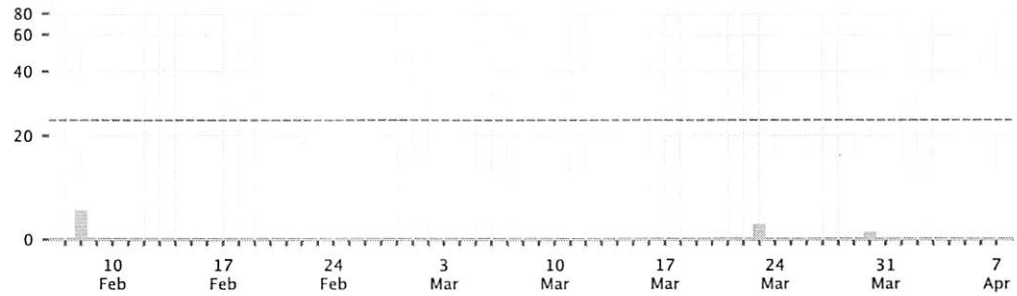

Pressure (cmH2O)

Mode **AutoSet**
 Set EPR **Fulltime, 3.0**
 Set Max Pressure **18.0**
 Set Min Pressure **7.0**
 Maximum (avg) **16.4**
 95th % (avg) **15.0**
 Median (avg) **10.6**

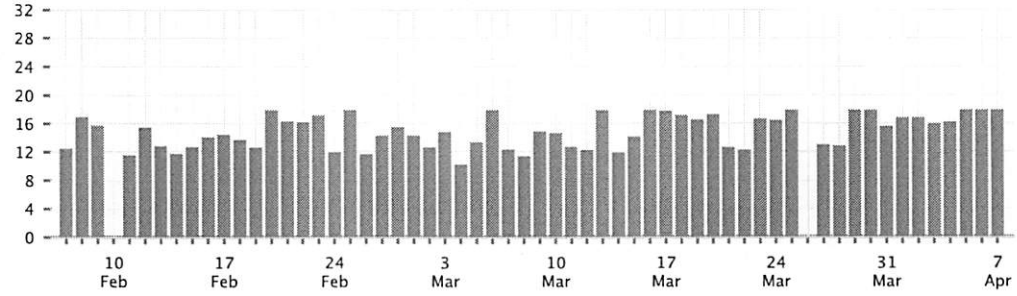

AHI (events/hour)

AHI
 HI
 AI
 CAI
 OAI
 UAI
 RERA
 CSR% (avg)

